



## Reference Material

This certificate is designed in accordance with ISO 17034 and ISO Guide 31. This reference material (RM) was designed, produced and verified in accordance with ISO/IEC 17025, ISO 17034 and a registered quality management system ISO 9001.

### Product Name

Chloroparaffin C10-C13, 63% Cl 100 µg/mL in Cyclohexane

Product Code	Lot Number
DRE-X23106300CY	G1230987CY
CAS No.	Format
85535-84-8	Solution
Mol. Weight	Expiry Date
	11 Jan 2028
Mol. Formula	Storage Temp
	20°C ± 4°C

### CERTIFIED

Concentration  
99.90 µg/mL

### CERTIFIED

Expanded Uncertainty (U)  
8.00 µg/mL

### Uncertainty


The certified value(s) and uncertainty(ies) are determined in accordance with ISO 17034 with an 95% confidence level (k=2). Uncertainty is based on the Total Combined Uncertainty, including uncertainties of preparation, purity of neat materials, homogeneity and stability testing. Stability values are based on real evidence opposed to simulation.

The producer certifies that this reference material meets the specification stated in this certificate until the expiry date, provided it is stored unopened at the recommended temperature herein. Product warranties for this reference material are set out in the terms and conditions of purchase.

CERTIFIED BY	CERTIFIED ON		
L. Messerschmid	11 Jan 2023		RM Release



## CHROMATOGRAM

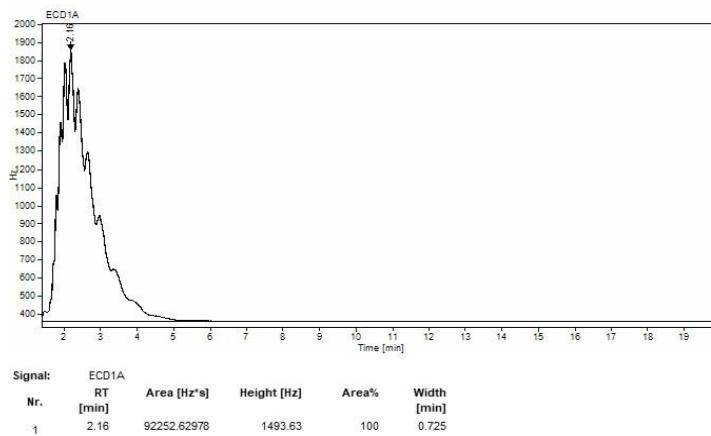

## Instrument

GC/ECD

## Detection

ECD

## Column

Optima-5MS, 0.25 µm, 0.25 mm

## Method Details

Initial Temp: 320°C / 20 min, End Temp: 320°C, Gradient: 0°C/min

## Inj.-Vol.

1.0 µL

## Flow

1 mL/min

## Method of Preparation

The certified value is based on gravimetric and volumetric preparation of this RM. This RM has been confirmed by the appropriate analytical techniques.

## Batch Information

Solvent: Cyclohexane, Lot No. 012022CR2, 2000.00 mL.

Mixture of Congeners.

## Gravimetric Data

Compound Name	Lot No.	Weight (mg)	Purity (%)
Chloroparaffin C10-C13, 63% Cl *	170504	199.997	99.9

\*mixture of congeners -- See Batch information

## Intended Use

This RM is intended for use in a laboratory as a calibration and quality control standard or in method development for analytical techniques.

the balances is verified daily internally and annually by an external accredited calibration service. Chromatographic methods are traceable to the International System of Units (SI).

## Instructions for use

The RM should be used shortly after opening to avoid concentration changes due to evaporation. It is recommended to use 1 mL as the minimum sample size and if less material is used, to increase the certified uncertainty by a factor of two for half sample and four for a quarter of sample. If storage after opening is necessary, the RM should be tightly closed and kept from light and moisture. If the RM was in a sealed ampoule, it should be transferred to a vial with minimum head space. Visit the support section of our website [lgcstandards.com](http://lgcstandards.com) for a series of Dr. Ehrenstorfer Tech Tip videos and frequently asked questions.

## Safety

Proper precautions should be observed while handling. See Safety Data Sheet.

## Homogeneity

Random replicate samples of the final packaged RM have been analysed to prove homogeneity compliant with ISO 17034.

## Traceability

The balances used for gravimetric measurements are calibrated with weights traceable to the national standards (DKD). The calibration of

## Storage

The RM should be stored in the original sealed container at the indicated temperature.